



Certificado No.:

42801

Registrador de Temperatura y Humedad

Fecha de Calibración:

2024-02-20

Maxim / Honeywell

**NO VALIDO**

Tabla 1.0: Lecturas de la TEMPERATURA en el área de trabajo (°C)

Tiempo (hh:mm:ss)	Temperatura Patrón (°C)	Temperatura Calibrando (°C)	Error (°C)
9:15:00 AM	17.8	17.6	-0.2
9:15:30 AM	17.8	17.5	-0.3
9:16:00 AM	17.5	17.3	-0.2
9:16:30 AM	17.3	17.1	-0.2
9:17:00 AM	17.3	17.0	-0.3
9:17:30 AM	16.8	16.5	-0.3
9:18:00 AM	16.8	16.4	-0.4
9:18:30 AM	16.3	16.4	0.1
9:19:00 AM	16.1	16.3	0.2
9:19:30 AM	15.9	16.1	0.2
9:20:00 AM	15.6	15.9	0.3
9:20:30 AM	15.2	15.6	0.4
9:21:00 AM	14.8	15.0	0.2
9:21:30 AM	14.5	14.8	0.3
9:22:00 AM	14.1	14.4	0.3
9:22:30 AM	13.9	14.1	0.2
9:23:00 AM	13.6	13.9	0.3
9:23:30 AM	13.4	13.6	0.2
9:24:00 AM	13.0	13.3	0.3
9:24:30 AM	12.7	13.1	0.4
9:25:00 AM	12.4	12.8	0.4
9:25:30 AM	12.1	12.4	0.3
9:26:00 AM	11.8	12.1	0.3
9:26:30 AM	11.4	11.8	0.4
9:27:00 AM	11.0	11.3	0.3
9:27:30 AM	10.8	11.1	0.3
9:28:00 AM	10.5	10.9	0.4
9:28:30 AM	10.2	10.5	0.3
9:29:00 AM	9.8	10.2	0.4
9:29:30 AM	9.4	9.7	0.3
<b>Promedio</b>	<b>14.0</b>	<b>14.2</b>	
<b>Desviación</b>	<b>2.643</b>	<b>2.448</b>	
<b>Max</b>	<b>17.8</b>	<b>17.6</b>	
<b>Min</b>	<b>9.4</b>	<b>10.2</b>	

**PAGO PENDIENTE**

Certificado No.:

42801

Registrador de Temperatura y Humedad

Fecha de Calibración:

2024-02-20

Maxim / Honeywell

**NO VALIDO**

Tabla 2.0: Lecturas de la HUMEDAD RELATIVA en el área de trabajo (%HR)

Tiempo (hh:mm:ss)	Humedad Relativa Patrón (%HR)	Humedad Relativa Calibrando (%HR)	Error (%HR)
9:15:00 AM	58.8	58.59	-0.2
9:15:30 AM	59.3	59.74	0.4
9:16:00 AM	58.1	57.83	-0.3
9:16:30 AM	58.8	58.61	-0.2
9:17:00 AM	59.4	59.67	0.3
9:17:30 AM	60.9	61.35	0.5
9:18:00 AM	61.2	61.56	0.4
9:18:30 AM	61.6	61.78	0.2
9:19:00 AM	61.9	62.23	0.3
9:19:30 AM	62.5	62.61	0.1
9:20:00 AM	63.0	62.98	0.0
9:20:30 AM	63.3	63.45	0.2
9:21:00 AM	63.6	63.88	0.3
9:21:30 AM	64.2	64.12	-0.1
9:22:00 AM	64.5	64.32	-0.2
9:22:30 AM	64.9	64.83	-0.1
9:23:00 AM	65.3	65.12	-0.2
9:23:30 AM	65.7	65.44	-0.3
9:24:00 AM	66.1	65.81	-0.3
9:24:30 AM	66.3	66.24	-0.1
9:25:00 AM	66.7	66.59	-0.1
9:25:30 AM	67.2	66.97	-0.2
9:26:00 AM	67.5	67.15	-0.3
9:26:30 AM	67.8	67.61	-0.2
9:27:00 AM	68.3	68.09	-0.2
9:27:30 AM	68.7	68.96	0.3
9:28:00 AM	69.1	69.24	0.1
9:28:30 AM	69.4	69.76	0.4
9:29:00 AM	69.9	70.22	0.3
9:29:30 AM	70.4	70.76	0.4
<b>Promedio</b>	<b>64.5</b>	<b>64.5</b>	
<b>Desviación</b>	<b>3.657</b>	<b>3.652</b>	
<b>Max</b>	<b>70.4</b>	<b>70.2</b>	
<b>Min</b>	<b>58.1</b>	<b>57.8</b>	

Certificado No.:

42801



Registrador de Temperatura y Humedad

Fecha de Calibración:

2024-02-20

Maxim / Honeywell

**NO VALIDO**

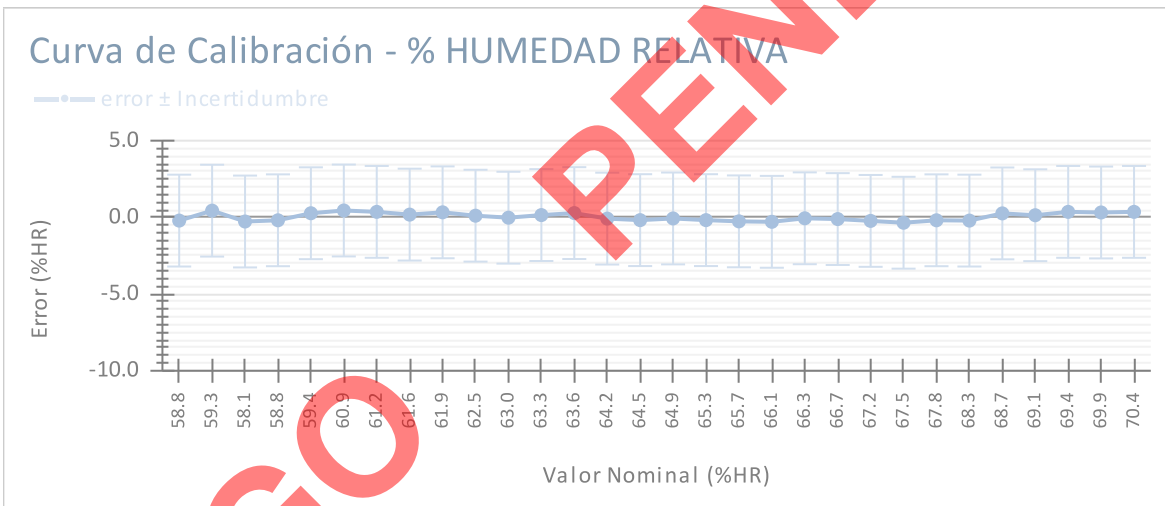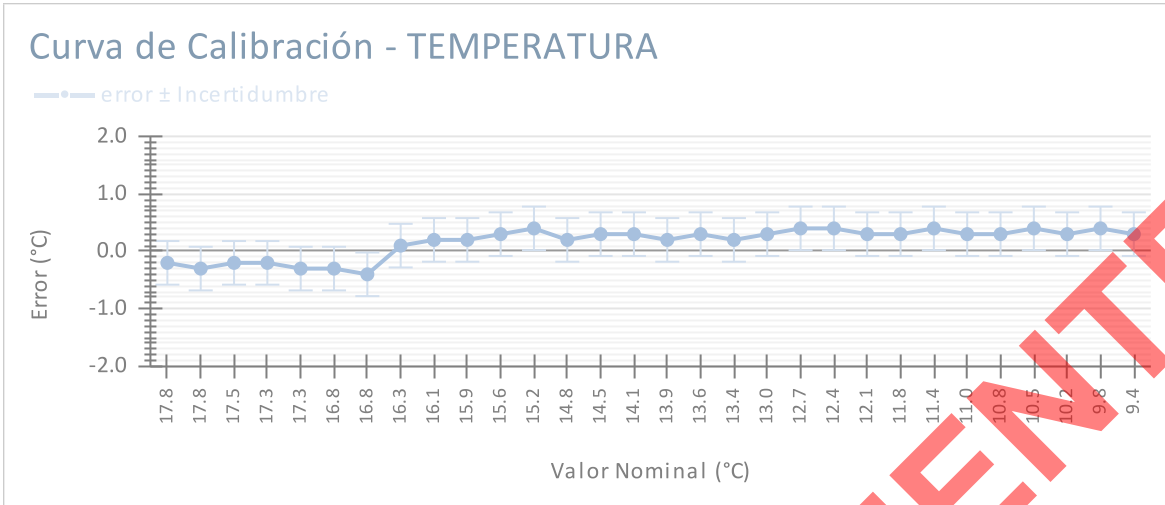

**PAGO PENDIENTE**