



Certificado No.:

66782

Controlador de Temperatura

Fecha de Calibración:

2026-03-03

QUECLINCK

Tabla 1.0: Lecturas de la TEMPERATURA en el área de trabajo (°C)

Tiempo (hh:mm:ss)	Temperatura Patrón (°C)	Temperatura Calibrando (°C)	Error (°C)
11:40:00 AM	0.2	0.6	0.40
11:41:00 AM	0.5	0.7	0.20
11:42:00 AM	0.9	1.0	0.10
11:43:00 AM	1.1	1.3	0.20
11:44:00 AM	1.3	1.6	0.30
11:45:00 AM	1.5	1.7	0.20
11:46:00 AM	1.8	2.0	0.20
11:47:00 AM	2.0	2.1	0.10
11:48:00 AM	2.1	2.4	0.30
11:49:00 AM	1.9	2.5	0.60
11:50:00 AM	1.1	2.2	1.10
11:51:00 AM	0.2	1.5	1.30
11:52:00 AM	-0.1	0.8	0.90
11:53:00 AM	-0.5	0.4	0.90
11:54:00 AM	-0.6	0.1	0.70
11:55:00 AM	-0.6	0.0	0.60
11:56:00 AM	-0.6	0.0	0.60
11:57:00 AM	-0.7	-0.3	0.40
11:58:00 AM	-0.7	-0.2	0.50
11:59:00 AM	-0.8	-0.3	0.50
12:00:00 PM	-0.8	-0.5	0.30
12:01:00 PM	-0.8	-0.5	0.30
12:02:00 PM	-0.9	-0.6	0.30
12:03:00 PM	-1.1	-0.7	0.40
12:04:00 PM	-1.2	-0.9	0.30
12:05:00 PM	-1.3	-1.0	0.30
12:06:00 PM	-1.3	-1.1	0.20
12:07:00 PM	-1.5	-1.3	0.20
12:08:00 PM	-1.8	-1.6	0.20
12:09:00 PM	-2.1	-1.9	0.20
<b>Promedio</b>	<b>-0.09</b>	<b>0.3</b>	
<b>Desviación</b>	<b>1.224</b>	<b>1.265</b>	
<b>Max</b>	<b>2.10</b>	<b>2.50</b>	
<b>Min</b>	<b>-2.10</b>	<b>-1.60</b>	

# NO VALIDO

Certificado No.:


66782

Controlador de Temperatura

Fecha de Calibración:

2026-03-03

QUECLINCK

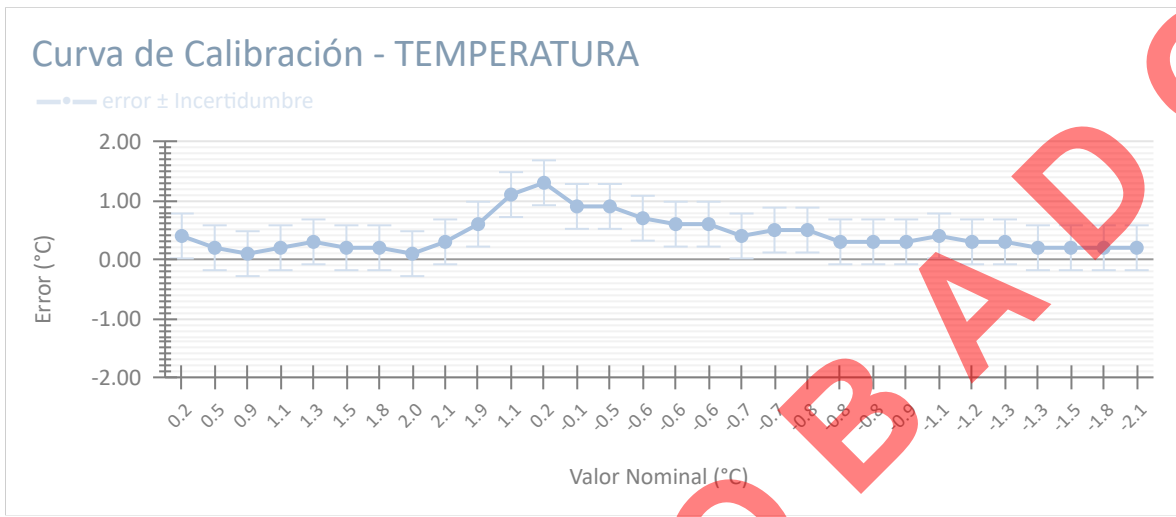

NO APROBADO