

Certificado No.:


67152

Registrador de Temperatura y Humedad

Fecha de Calibración:

2026-03-14

Queclink

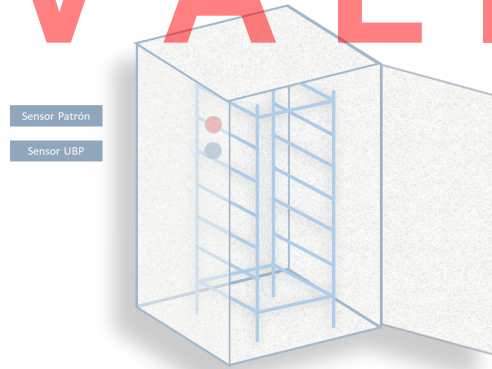

UBICACION DE EQUIPOS PATRON

Tabla 1.0: Lecturas de la TEMPERATURA en el área de trabajo (°C)

Tiempo (hh:mm:ss)	Temperatura Patrón (°C)	Temperatura Calibrando (°C)	Error (°C)
10:15:00 AM	17.80	17.10	-0.70
10:17:00 AM	17.50	16.50	-1.00
10:19:00 AM	17.10	16.20	-0.90
10:21:00 AM	17.00	16.10	-0.90
10:23:00 AM	16.80	16.00	-0.80
10:25:00 AM	16.50	15.80	-0.70
10:27:00 AM	16.20	15.40	-0.80
10:29:00 AM	16.00	15.20	-0.80
10:31:00 AM	16.00	15.00	-1.00
10:33:00 AM	15.80	15.00	-0.80
10:35:00 AM	15.40	14.20	-1.20
10:37:00 AM	15.40	14.70	-0.70
10:39:00 AM	15.10	14.80	-0.30
10:41:00 AM	15.00	13.00	-2.00
10:43:00 AM	15.00	13.50	-1.50
10:45:00 AM	14.80	13.80	-1.00
10:47:00 AM	14.90	13.90	-1.00
10:49:00 AM	14.70	13.40	-1.30
10:51:00 AM	14.20	13.80	-0.40
10:53:00 AM	14.10	13.90	-0.20
10:55:00 AM	14.00	14.00	0.00
10:57:00 AM	13.80	14.10	0.30
10:59:00 AM	13.40	14.20	0.80
11:01:00 AM	13.50	14.50	1.00
11:03:00 AM	13.80	14.80	1.00
11:05:00 AM	14.00	14.90	0.90
11:07:00 AM	14.21	15.10	0.89
11:09:00 AM	14.10	15.10	1.00
11:11:00 AM	14.80	15.40	0.60
11:13:00 AM	14.90	15.80	0.90
Promedio	15.19	14.84	
Desviación	1.23	1.00	
Max	17.80	17.10	
Min	13.40	13.00	

Certificado No.:

67152

Registrador de Temperatura y Humedad

Fecha de Calibración:

2026-03-14

Queclink

Tabla 2.0: Lecturas de la HUMEDAD RELATIVA en el área de trabajo (%HR)

Tiempo (hh:mm:ss)	Humedad Relativa Patrón (%HR)	Humedad Relativa Calibrando (%HR)	Error (%HR)
10:15:00 AM	68.10	66.20	-1.90
10:17:00 AM	68.10	66.10	-2.00
10:19:00 AM	68.40	65.80	-2.60
10:21:00 AM	68.10	65.40	-2.70
10:23:00 AM	67.50	65.20	-2.30
10:25:00 AM	67.10	65.00	-2.10
10:27:00 AM	67.40	64.20	-3.20
10:29:00 AM	67.80	64.80	-3.00
10:31:00 AM	68.10	64.70	-3.40
10:33:00 AM	68.20	64.90	-3.30
10:35:00 AM	68.50	64.00	-4.50
10:37:00 AM	68.90	64.00	-4.90
10:39:00 AM	69.00	63.50	-5.50
10:41:00 AM	69.40	63.70	-5.70
10:43:00 AM	69.10	63.80	-5.30
10:45:00 AM	69.20	63.20	-6.00
10:47:00 AM	68.40	63.00	-5.40
10:49:00 AM	68.50	63.00	-5.50
10:51:00 AM	68.20	62.80	-5.40
10:53:00 AM	68.00	62.90	-5.10
10:55:00 AM	67.80	62.70	-5.10
10:57:00 AM	67.50	63.00	-4.50
10:59:00 AM	67.30	63.10	-4.20
11:01:00 AM	67.00	63.50	-3.50
11:03:00 AM	66.80	63.70	-3.10
11:05:00 AM	66.50	63.90	-2.60
11:07:00 AM	66.40	64.00	-2.40
11:09:00 AM	66.20	64.50	-1.70
11:11:00 AM	66.10	64.80	-1.30
11:13:00 AM	66.00	64.90	-1.10
Promedio	67.79	64.14	
Desviación	0.95	1.01	
Max	69.40	66.20	
Min	66.00	62.70	

Certificado No.:

67152



Registrador de Temperatura y Humedad

Fecha de Calibración:

2026-03-14

QuecLink

NO VALIDO

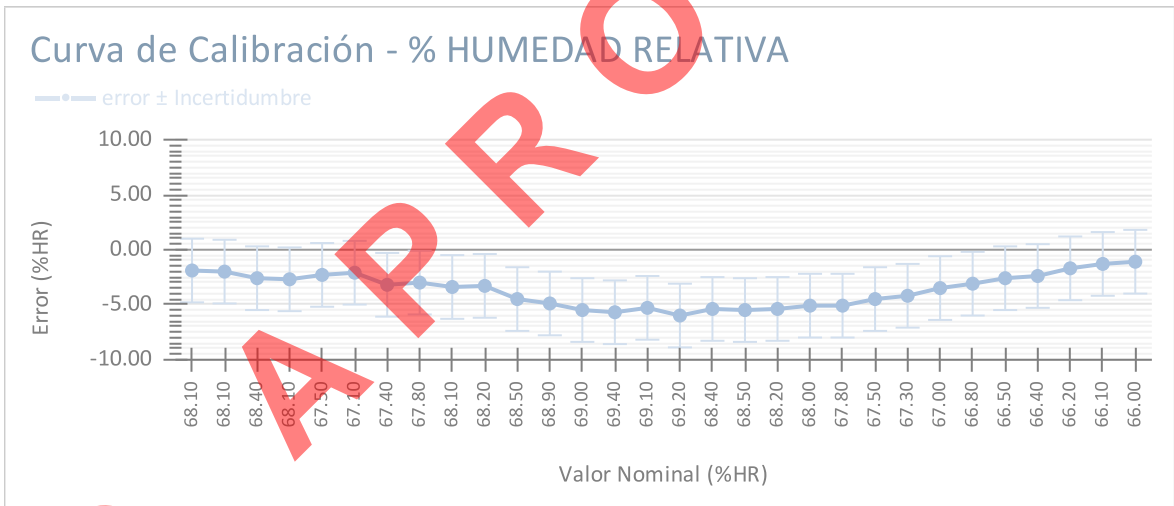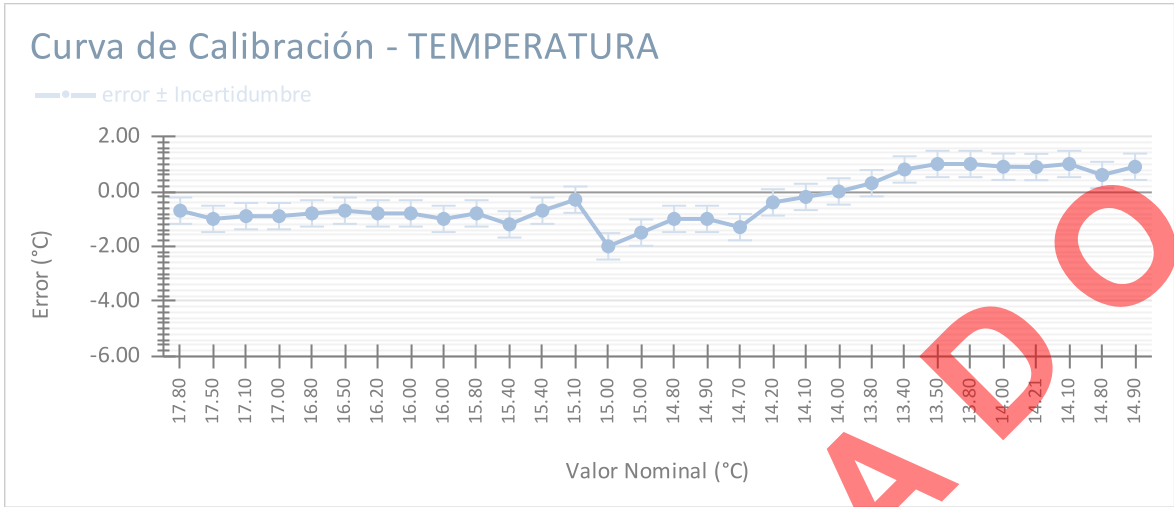

NO APROBADO